

Adenosine Analysis In Functional Cosmetic

1. Analytical Condition

YL 9100 Series QC Analyzer


Column : C18 (4.6 X 250mm, 5 μ m)

Detector : UV/Vis 260nm

Injection Volume : 20 μ l

Mobile Phase : Aqueous Solution(10mM Na₂HPO₄ + 10mM NaH₂PO₄)

Flow Rate : 1ml/min

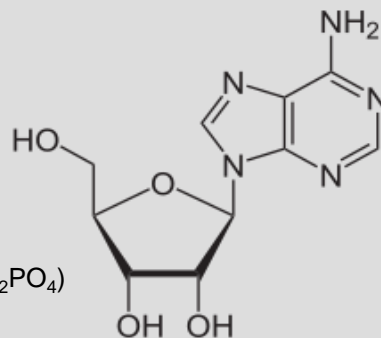

2. Chromatogram

